


Develosil Application Data

No.074 Carotenes in carrots/にんじん中のカロテン類

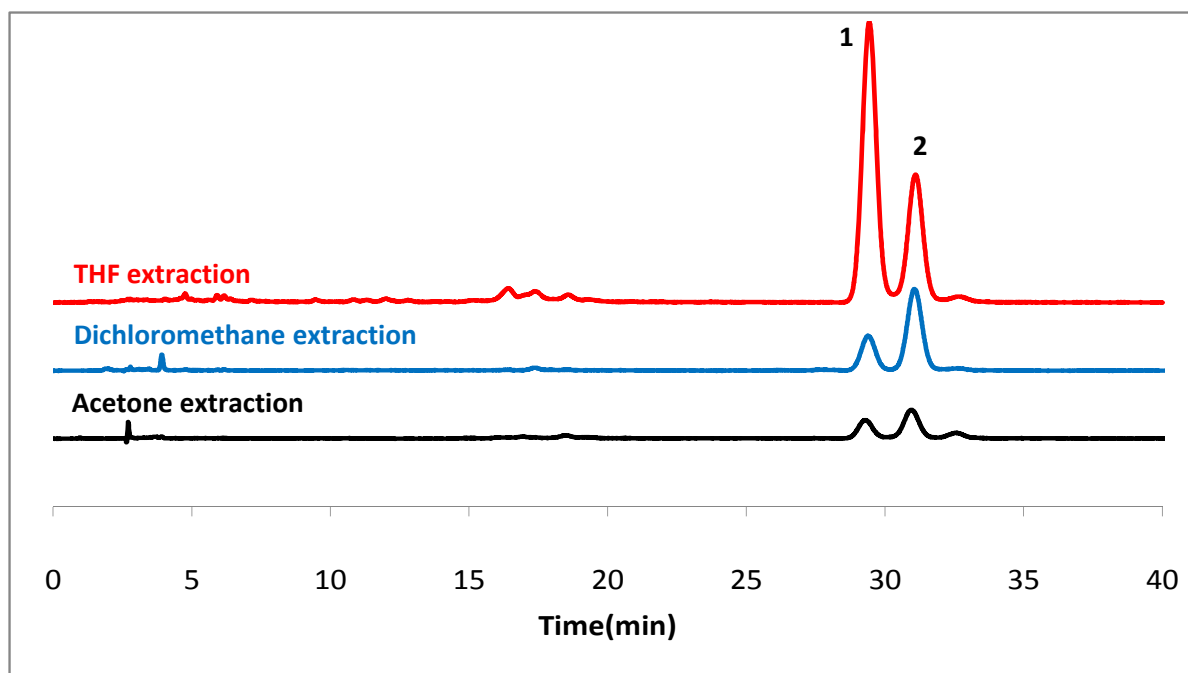

Analytical Conditions:

Column: Develosil HSR C18,5um (4.6x250mm)

Mobile phase: Methanol/Ethanol=90/10

Flow rate: 1.0mL/min

Temperature: 40°C

Detection: UV450nm

Sample: 1.α-Carotene

2.β-Carotene

Injection volume: 5.0uL

System: JASCO 2000series

